


# Signature Personalized Patient Care\*

## Surgical Technique Addendum

Oxford Partial Knee  
Microplasty Instrumentation

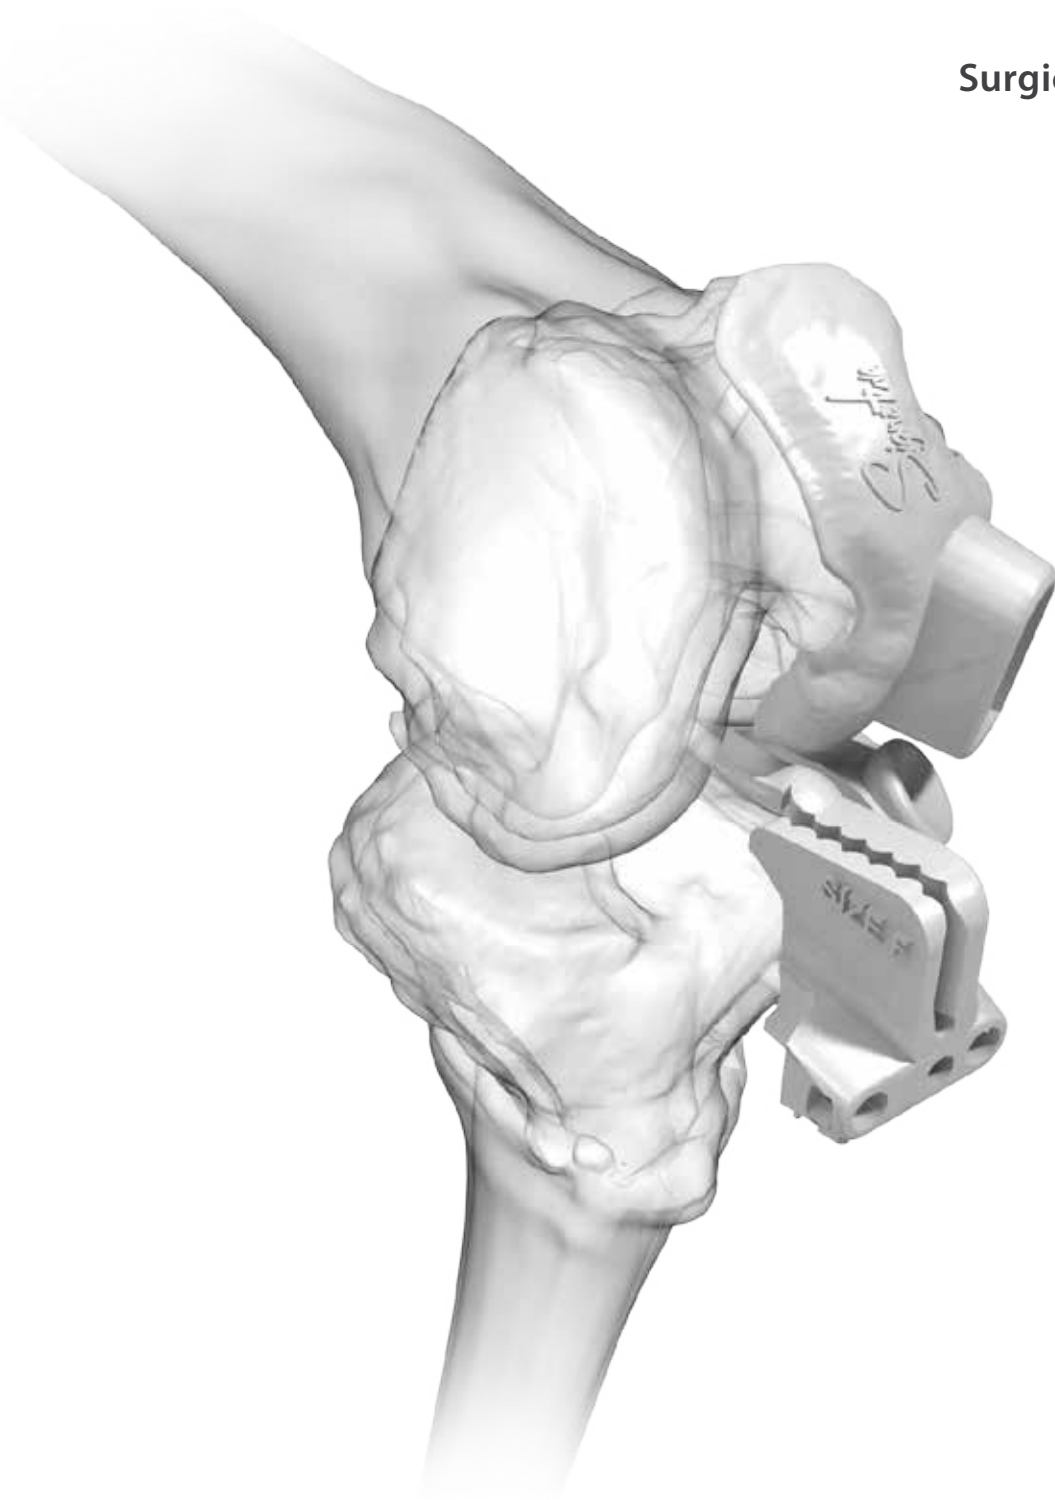

**BIOMET**

## One Surgeon. One Patient.

**Over 1 million times per year, Biomet helps one surgeon provide personalized care to one patient.**

The science and art of medical care is to provide the right solution for each individual patient. This requires clinical mastery, a human connection between the surgeon and the patient, and the right tools for each situation.

At Biomet, we strive to view our work through the eyes of one surgeon and one patient. We treat every solution we provide as if it's meant for a family member.

Our approach to innovation creates real solutions that assist each surgeon in the delivery of durable personalized care to each patient, whether that solution requires a minimally invasive surgical technique, advanced biomaterials or a patient-matched implant.

**When one surgeon connects with one patient to provide personalized care, the promise of medicine is fulfilled.**

# Signature Personalized Patient Care

---

## Contents

Positioning the Limb..... 4

Incision ..... 4

Soft Tissue Assessment ..... 5

Signature Femoral Guide Registration..... 9

Femoral Saw Cut ..... 11

First Milling of the Condyle ..... 12

Signature Tibial Guide Registration and Resection ..... 13

Ordering Information ..... 19

In addition to the Oxford Partial Knee this surgical technique addendum may also be used for the medial Vanguard M Partial Knee.

# Signature Personalized Patient Care

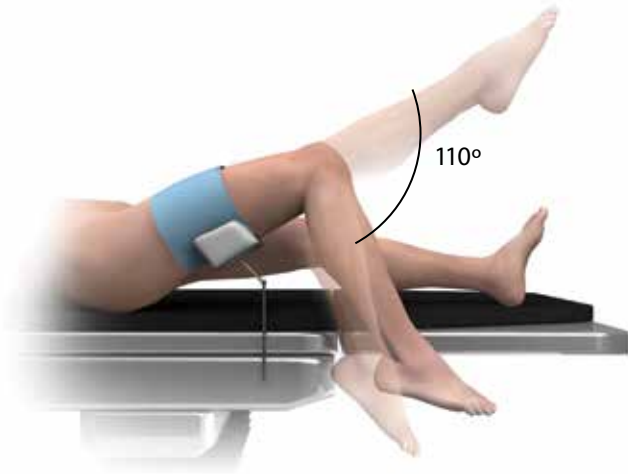


Figure 1



Figure 2

## Positioning the Limb

Inflate a thigh tourniquet and place the draped leg on a thigh support, with the hip flexed to about 30 degrees and the leg dependent. The knee must be free to flex fully and the leg should hang with the knee flexed about 110 degrees. The thigh support must not be placed in the popliteal fossa as this will increase the risk of damage to the popliteal vessels (Figure 1).

## Incision

With the knee flexed to 90 degrees, make a medial parapatellar skin incision from the medial margin of the patella to a point 3 cm distal to the joint line (Figure 2). Deepen the incision through the joint capsule. At its upper end, the capsular incision should extend proximally about 2 cm into the vastus medialis.

This surgical technique is utilized by Mr. Chris Dodd, F.R.C.S., Roger Emerson Jr., M.D., Adolph Lombardi Jr., M.D., David Mauerhan, M.D. and Prof. David Murray, F.R.C.S. Biomet as the manufacturer of medical devices does not practice medicine. Each surgeon is responsible for determining the appropriate device, technique(s) and product(s) to utilize on each individual patient.

It should pass around the patella and down beside the patella tendon. The anterior surface of the medial tibial plateau should be exposed.

Excise part of the retropatellar fat pad and insert retractors into the synovial cavity. The ACL can now be inspected to ascertain that it is intact. (Absence of a functioning ACL is a contraindication. If this is found, the operation should be abandoned in favor of a total knee replacement).

**Note:** The Signature femoral and tibial partial knee arthroplasty (PKA) guides were designed to register off the osteophytes. Therefore, do not remove the osteophytes.

**Note:** The MRI-based Signature femoral and tibial PKA guides were designed to replicate the preoperative surgeon-approved plan. Final component position should be validated intraoperatively when the capsular soft tissues may be appropriately assessed.



Figure 3

## Soft Tissue Assessment

Signature software plans the femur and tibia independently and does not assess soft tissue. The Oxford Partial Knee is a soft tissue procedure and it is critical that the soft tissue is assessed by using the Oxford Microplasty 1 mm femoral sizing spoon.

With the knee in flexion, insert the appropriate 1 mm femoral sizing spoon (based on pre-operative Signature plan) centrally in the medial compartment (Figure 3). Femoral size can be confirmed by examining the relationship of the front of the spoon and an estimate of where the cartilage surface would have been before the arthritis.

Once femoral size is confirmed, ensure all retraction is removed and assess the ligament tension with the femoral sizing spoon. If the femoral sizing spoon achieves appropriate ligament tension, ensure the 0 mm shim is used when making the tibial resection.

**Note: If the spoon is loose, then the +2 mm shim should be utilized when making the tibial resection.**

# Signature Personalized Patient Care



Figure 4



Figure 5

## Signature Femoral Guide Registration

**Note:** The Signature femoral guide was designed to register on the osteophytes. Therefore, do not remove the osteophytes prior to guide placement.

Flex the knee to 90 degrees. Using methylene blue, draw a line down the center of the medial condyle.

With the knee in extension, place the Signature femoral guide under the incision and quad tendon anteriorly past the point of planned registration. Rotate the guide posteriorly then laterally, while flexing the knee to approximately 90 degrees.

**Note:** Flexing beyond 90 degrees may cause the patella tendon to force the guide out of position. If necessary, use a patella retractor and/or decrease amount of flexion to allow for proper fit.

Register the guide in a fluid motion from anterior to posterior, then medial to lateral to lock the guide onto the medial condyle, condylar notch and the anterior medial ridge. The guide should register flush against exposed bone and cartilage without soft tissue impingement. Validate proper registration utilizing the drill guide window. This can be confirmed by looking into the drill guide window and verifying the position of the line. If the line is not central adjust the guide position (Figure 4). Additionally, retractors may be used to assess guide registration peripherally.

Once proper registration is achieved, insert the appropriate size femoral drill guide into the Signature femoral PKA guide (Figure 5). Only the appropriately sized femoral drill guide will fit properly within the Signature guide. When seated properly, only the top etched line on the tapered portion of the drill guide should be visible.



Figure 6

## Signature Femoral Guide Registration (cont.)

**Note:** Varus/valgus and flexion alignment can be evaluated before drilling by sliding the femoral alignment checker onto the femoral drill guide and inserting an EM rod through the alignment hole (Figure 6). If indicated alignment does not match the plan or is unacceptable, Do Not Drill. This could indicate improper guide registration. Check for proper guide registration or revert to standard instrumentation to complete surgical technique.

Pass the 4 mm drill through the anterior hole. Drill into the bone to its depth stop. Leave the 4 mm drill in place and advance the 6 mm drill through the posterior hole in the femoral drill guide until its depth stop. Remove the 4 and 6 mm drills, femoral drill guide and the Signature femoral PKA guide from the joint.



Figure 7



Figure 8

## Femoral Saw Cut

Insert the posterior resection guide into the drilled holes and tap home (Figure 7).

Insert a retractor to protect the MCL. Using the 12 mm broad sagittal saw, excise the posterior facet of the femoral condyle. The saw blade should be bent slightly by dropping the saw to ensure it is guided by the underside of the posterior resection guide (Figure 8). Take care to avoid damage to the medial collateral and anterior cruciate ligaments.

Remove the guide with the slap hammer, taking care not to distort the drill holes. Remove the bone fragment.

There is now good access to the back of the joint, and any remnants of the medial meniscus should be removed. In the region of the MCL, a small cuff of meniscus should be left to protect the MCL from the tibial component. The posterior horn should be completely removed.





Figure 9



Figure 10



Figure 11

## First Milling of the Condyle

Insert the 0 spigot, which has the thickest flange, into the large posterior drill hole and tap it until the flange abuts against the bone (Figure 9).

**Note:** The 0 spigot is designed to remove sufficient bone to allow the femoral component to seat. This amount varies with the degree of arthritic erosion of the condyle.

By extending the knee slightly and retracting the soft tissues, maneuver the spherical cutter onto the spigot (Figure 10) and into the wound so that the teeth touch the bone (Figure 11). Take care to avoid trapping soft tissues.

When milling, push firmly in the direction of the spigot axis, taking care not to tilt the tool. Mill until the cutter will no longer advance.

**If in doubt, continue to mill.  
There is no risk of over-milling.**



Figure 12

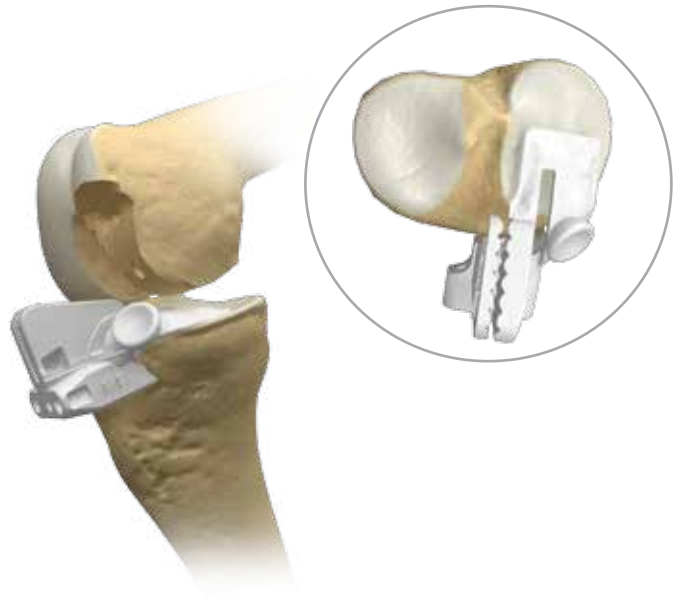


Figure 13

Remove the mill and the spigot and trim off the bone protruding from the posterior corners of the condyle that lie outside the periphery of the cutting teeth (Figure 12). Do not damage the flat posterior surface of the condyle.

All osteophytes may now be removed from the medial margin of the medial femoral condyle and from both margins of the intercondylar notch. The assistant extends and flexes the knee, moving the incision up and down, allowing the various osteophytes to come into view.

With a narrow chisel (6 mm), remove the osteophytes from beneath the medial collateral ligament and from the posterolateral margin of the medial condyle.

**Note:** No further milling should be performed until the tibial preparation is complete.

## Signature Tibial Guide Registration and Resection

Expose the front of the tibia in the lower part of the wound from the tibial tubercle to the rim of the plateau.

**Note:** Do not 'release' any of the fibers of the medial collateral ligament.

**Note:** The Signature tibial partial knee arthroplasty (PKA) guides were designed to register off the osteophytes. Therefore, do not remove the osteophytes.

**Note:** The MRI-based Signature femoral and tibial PKA guides were designed to replicate the preoperative surgeon-approved plan. Final component position should be validated intraoperatively when the capsular soft tissues may be appropriately assessed.

Register the Signature tibial PKA guide onto the medial plateau and rotate downward until the guide makes contact anteriorly (Figure 13). The pressure point on the tibial guide can be used to aid in proper registration of the tibial PKA guide. Slight pressure can be applied to the pressure point on the anteromedial part of the guide.



Figure 14



Figure 15

Insert the tibial drill guide into the Signature tibial PKA guide (Figure 14). Signature tibial guide position may be validated by utilizing the guide window to assess plateau coverage and evaluate fit.

**Note:** Varus/valgus and slope alignment can be validated prior to drilling by sliding the tibial alignment checker onto the lateral side of the drill guide and inserting a rod through the alignment hole (Figure 15). If indicated alignment does not match plan the or is unacceptable, **Do Not Drill**. This could indicate improper guide registration. Check for proper guide registration or revert to standard instrumentation to complete surgical technique.



Figure 16



Figure 17

## If Ligament Tension was Achieved with 1 mm Femoral Sizing Spoon

If the 1 mm femoral sizing spoon achieved proper ligament tension, drill a 1/8" trochar pin into the pin hole at the base of the vertical cut slot in the Signature patient-specific tibial PKA guide.

Pass 1/8" drill pins through two of the remaining taper holes in the Signature tibial guide (Figure 16).

Insert the saw blade into the cut slot before engaging power. Use a reciprocating saw to make the vertical tibial cut. Advance the saw vertically through the cut slot on the Signature tibial PKA guide down until it rests on the surface of the 1/8" drill (Figure 17). The pin will act as a saw stop.

Remove the 1/8" drill from the pin hole at the base of the vertical cut slot, drill guide and Signature tibial guide. The two distal pins should be left in place.



Figure 18



Figure 19



Figure 20

## Signature Tibial Guide Registration and Resection (cont.)

Slide the tibial retractor onto the remaining 1/8" drill pins through the drilled pin holes. Once in position, validate varus/valgus and posterior slope alignment using tibial retractor (Figures 18 and 19).

Before making the horizontal cut, insert a medial collateral ligament (MCL) retractor. Ensure the retractor is between the saw and the MCL.

Use a 12 mm wide oscillating saw blade with appropriate markings to excise the plateau (Figure 20). Insert the captured or non-captured shim saw guide. Ensure the saw blade is run along the MCL retractor to completely cut the medial cortex. To cut the posterior cortex deepen the cut until the appropriate mark on the saw blade is aligned with the anterior cortex. After the tibial resection use pulse lavage to clear any debris.



Figure 21



Figure 22

## If Ligament Tension was **Not** Achieved with 1 mm Femoral Sizing Spoon

If the 1 mm femoral sizing spoon was loose, pass 1/8" drill pins through two of the taper holes in the Signature tibial guide (Figure 21).

**Do not drill a pin at the base of the vertical cut slot in the Signature patient-specific tibial PKA guide.** Instead, insert the reciprocating saw blade into the vertical cut slot. Score the tibial spine to orient the medial / lateral, as well as, tibial rotation of the vertical resection, however do not fully make the vertical resection (Figure 22).



Figure 23

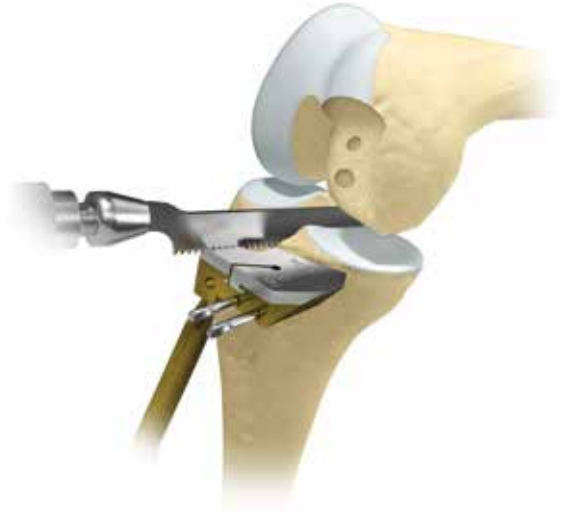


Figure 24

Remove the drill guide and Signature tibial guide. The two distal pins should be left in place.

With the +2 mm uncaptured tibial shim assembled to the tibial retractor, slide the tibial retractor onto the remaining 1/8" drill pins through the drilled pin holes. Once in position, validate varus/valgus and posterior slope alignment using the tibial retractor (Figure 23).

Using the reciprocating saw, complete the vertical resection using the scored cut made through the Signature patient-specific tibial PKA guide (Figure 24). Do not lift the saw handle as this will dip the saw blade and increase the risk of tibial plateau fracture.

Before making the horizontal cut, insert a medial collateral ligament (MCL) retractor. Ensure the retractor is between the saw and the MCL.

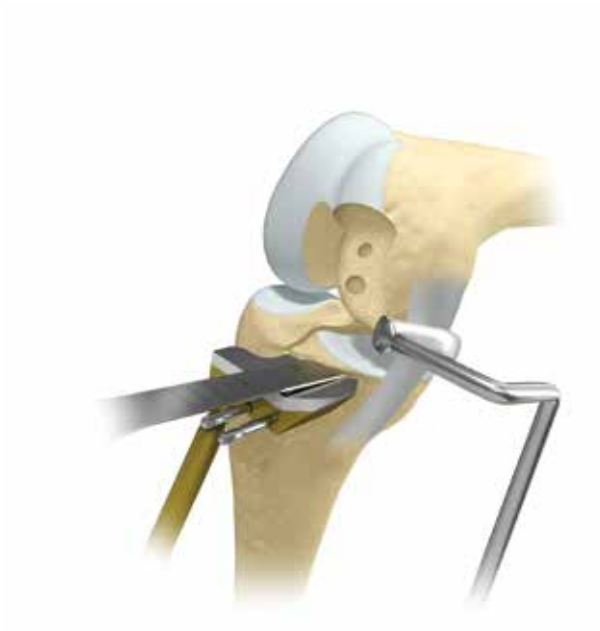


Figure 25

### If Ligament Tension was **Not** Achieved with 1 mm Femoral Sizing Spoon (cont.)

Use a 12 mm wide oscillating sawblade with appropriate markings to excise the plateau (Figure 25). Ensure the saw blade is run along the MCL retractor to completely cut the medial cortex.

To cut the posterior cortex deepen the cut until the appropriate mark on the saw blade is aligned with the anterior cortex. After the tibial resection use pulse lavage to clear any debris.





Figure 26

When the plateau is loose, lever it up with a broad osteotome and remove (Figure 26). Posterior soft tissue attachments may need to be cut with a knife. The posterior horn of the medial meniscus can now be removed.

The excised plateau will show the classic lesion of anteromedial osteoarthritis with eroded cartilage and bone in its mid and anterior parts and preserved cartilage posteriorly (Figure 27). Osteophytes around the edge of the plateau remain attached after its removal.



Figure 27

Use the excised plateau with the tibial templates to confirm the size of the tibial implant. Lay templates of the opposite side on the cut surface of the excised plateau to choose the component with the appropriate width.

Osteophytes on the tibial plateau in front of the insertion of the ACL and in the top of the notch must be removed to allow the fixed flexion deformity to correct. If there are large osteophytes around the patella they, should also be removed.

# Signature Personalized Patient Care

---



Figure 28

The thickness of bone removed from the tibia must be enough to accommodate the tibial template and a bearing at least 4 mm thick (3 mm is the smallest size available). To check that sufficient bone has been excised, insert the femoral trial, tibial template and a 4 mm gauge (Figure 28), this should be done at 100° of flexion.

**Note:** Whenever a feeler gauge is used to measure a gap, the retractors are removed. When left in, they have the effect of tightening the soft tissues, which artificially diminishes the gap.






If the 4 mm feeler gauge cannot be inserted or feels tight, more bone must be excised from the tibia. To do this, remove the initial/0 mm shim from the guide. Resect off the surface of the guide without shim to remove 2 mm of additional bone.

**Note:** If utilizing Phase III Instrumentation, shift the tibial resection guide from the bottom row of holes to the top row in order to remove 3 mm of additional bone.

After additional resection, recheck the gap with the tibial template in place and at least a 4 mm feeler gauge.

**See instrument platform surgical techniques for Equalizing and Confirming Flexion and Extension Gaps, Preventing Impingement, Final Preparation of the Tibial Plateau, Final Trial Reduction and Cementing the Components.**

## Instruments

Product	Part Number	Description	Size
	42-411400	Signature Alignment Rod	-
	42-411401	Signature Femoral Alignment Checker*	-
	42-411402 42-411403	Signature Tibial Alignment Checker (Left) Signature Tibial Alignment Checker (Right)	- -
	42-411420	Signature Tibial Drill Guide	-
 Downsize    Plan    Upsize	42-411430 42-411431 42-411434 42-411435 42-411436 42-411439 42-411440 42-411441 42-411444 42-411445 42-411446 42-411449 42-411450	Signature Femoral Drill Guide Signature Femoral Drill Guide (Upsize)* Signature Femoral Drill Guide (Downsize)* Signature Femoral Drill Guide Signature Femoral Drill Guide (Upsize)* Signature Femoral Drill Guide (Downsize)* Signature Femoral Drill Guide Signature Femoral Drill Guide (Upsize)* Signature Femoral Drill Guide (Downsize)* Signature Femoral Drill Guide Signature Femoral Drill Guide (Upsize)* Signature Femoral Drill Guide (Downsize)* Signature Femoral Drill Guide Signature Femoral Drill Guide (Upsize)* Signature Femoral Drill Guide (Downsize)* Signature Femoral Drill Guide	X-small Small X-small Small Medium Small Medium Large Medium Large Large X-large Large X-large

\* Optional to be used for intraoperative sizing if altering from approved Signature plan.

\*A collaborative partnership with Materialise N.V.

All trademarks herein are the property of Biomet, Inc. or its subsidiaries unless otherwise indicated.

This material is intended for the sole use and benefit of the Biomet sales force and physicians. It is not to be redistributed, duplicated or disclosed without the express written consent of Biomet.

For product information, including indications, contraindications, warnings, precautions and potential adverse effects, see the package insert herein and Biomet's website.

**BIOMET**  
ORTHOPEDICS

One Surgeon. One Patient.

©2014 Biomet Orthopedics • Form No. BMET0515.1 • REV0814

**Legal Manufacturer**  
Biomet Orthopedics  
P.O. Box 587  
56 E. Bell Drive  
Warsaw, Indiana 46581-0587  
USA

[www.biomet.com](http://www.biomet.com)

**Authorized Representative**  
Biomet UK, Ltd.  
Waterton Industrial Estate  
Bridgend, South Wales  
CF31 3XA  
UK

**Legal Manufacturer  
for Signature Guides**  
Materialise NV  
Technologilaan 15  
B-3001 Leuven  
Belgium

**CE0086**